
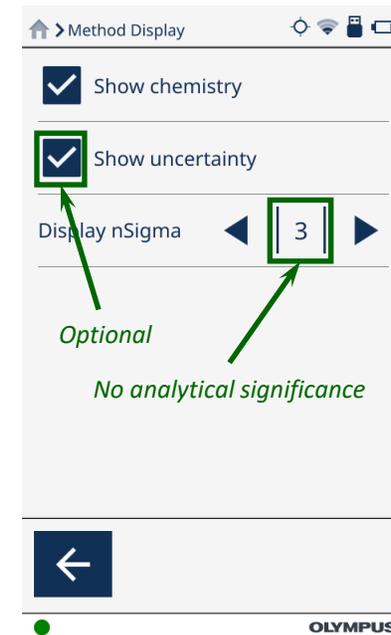
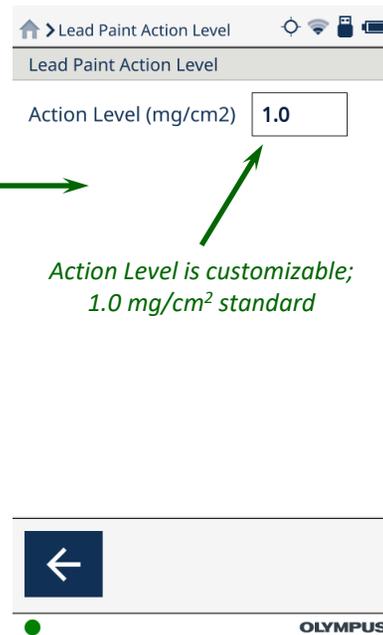
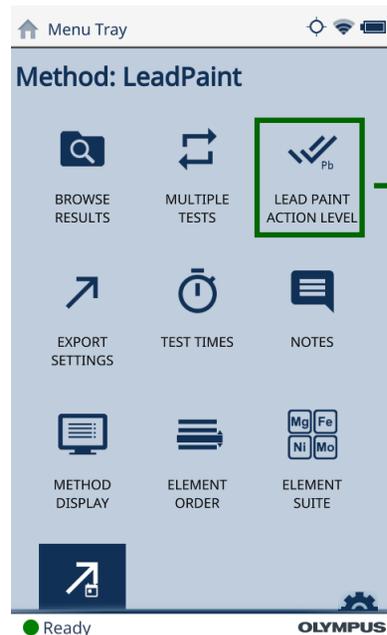
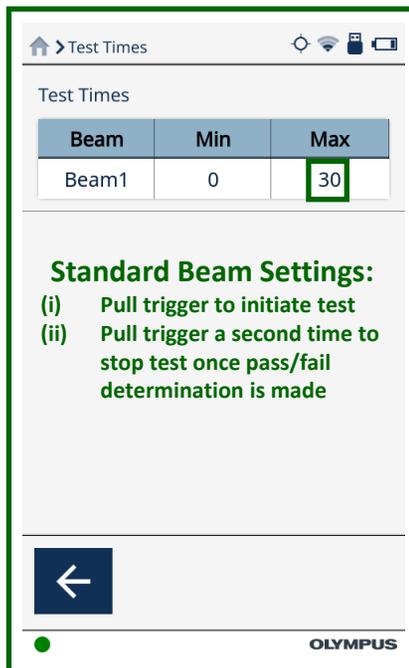
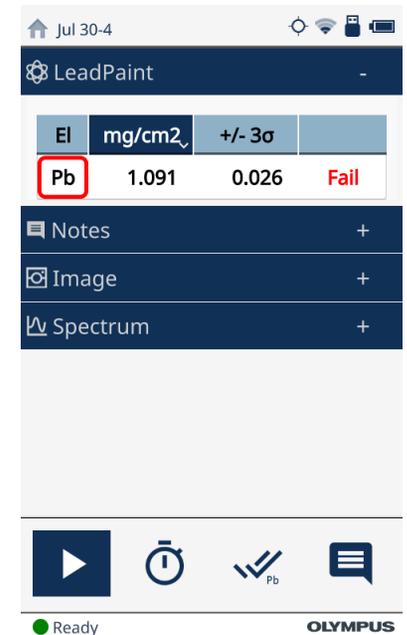


Lead Paint Getting Started Guide

- (1) Check your instrument window: Is the correct window installed? Is it intact? Clean it with an alcohol/wet wipe.
- (2) Check your Lead Paint Action Level setting. Default is 1.0 mg/cm²
- (3) Set your Test Time to 30 seconds
- (4) Check your Method Display Settings (bottom right).
- (5) Confirm that your collimator is turned off (back).
- (6) Select a useable Notes Template (back). Notes are optional but helpful for recording test-specific details.

NOTE: During testing, manually stop the test once a pass/fail determination has been made. This is typically 3-12 seconds. Leave your maximum test time longer in case it's needed. Stop the test by pulling the trigger a second time when the full time is not needed.

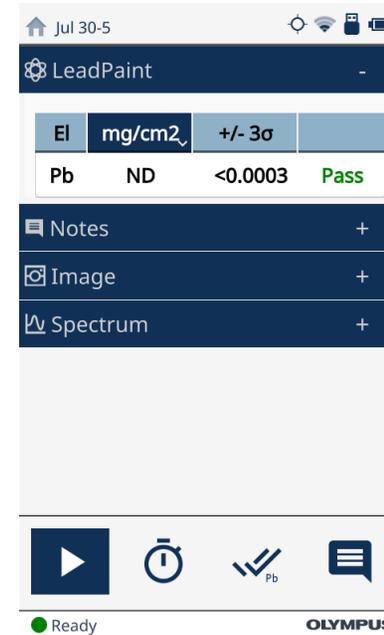

M-Series: Prolene



C-Series: Kapton Mesh



L-Series: Kapton ("Kap 50")

Lead Paint Getting Started Guide

Additional Online Resources:



[Quick Start Guide for Vanta M, C, and L Series Analyzers](#)



[Exporting Test Result to USB or SD Card](#)



[Creating a Custom Notes Template](#)



[Editing PDF Reporting Templates](#)

